



RUCK®
FÜR FUSS UND PFLEGE

PODOLOGSONIC



Compact instructions | REV 8 | Print

| REF 8011802




Dear customer,

You have decided to buy a device from the PODOLOG SONIC series. New design – new ideas – proven technology. Simple operation and maximum efficiency were the criteria and the result is impressive: For all devices, you can control all functions with just one rotary knob. Enormous time savings due to simultaneous cleaning and disinfection in just five minutes. SweepTec

technology for even ultrasonic distribution in the bath and thus a better cleaning result. Housing, oscillating bath and instrument basket made of stainless steel. Extended RUCK warranty of 3 years. All devices are approved as Class 1 medical products. The PODOLOG SONIC series offers a maximum of quality "made in Germany". We sincerely thank you for the trust

you have placed in our company and extend our best wishes for satisfaction in your daily work with our product. Please take some time to carefully read through the accompanying operating instructions from Bandelin before setting up the product and keep them in a safe place.

Kind regards, HELLMUT RUCK GmbH

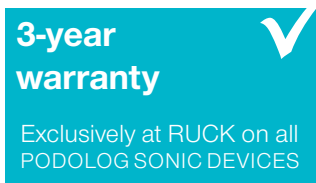

Class 1 medical product

Ultrasonic bath	Oscillating bath internal dimensions (L × W × D)	Work fill capacity	Ultrasonic peak power*/HF power	Weight (net)	Current consumption (230 V)	Fuses
	mm	l	W/Weff	kg	A	
Podolog S	190 × 85 × 60	0.6	160/40	2.2	0.2	T1A
Podolog M	240 × 140 × 100	2.0	320/80	3.4	0.4	F2A
Podolog XL	300 × 240 × 65	2.5	560/140	5.5	0.7	F2A

*To improve the effect, the ultrasound is modulated, resulting in a 4-fold value of the HF power as the ultrasonic peak power.

Compact instructions

(Please read the complete instructions from Bandelin, which are included in the scope of delivery.)

Illustration on the unit


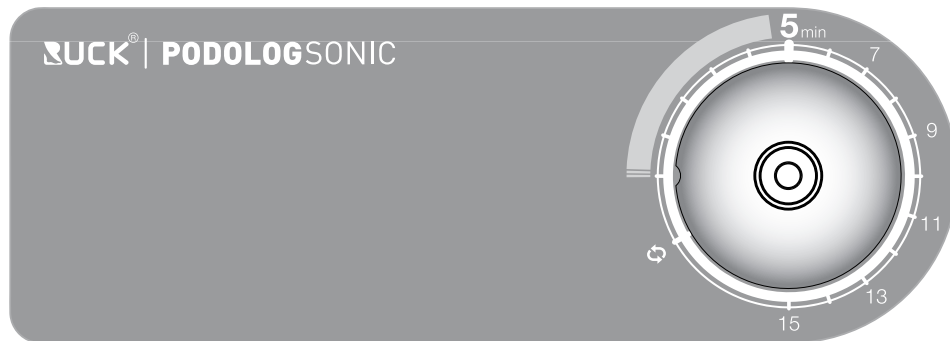


Illustration in the accompanying operating instructions from BANDELIN



01 Cleaning duration

In general, the cleaning duration should be set for as little time as possible. Depending on the degree of soiling and the cleaner fluid used (observe the information on the respective labels), the cleaning duration is between approx. 1 to 15 min.

02 Continuous operation setting ∞ / ↻:

- Engage rotary knob at the symbol ∞ / ↻.
- Device does not switch off automatically. To turn it off, move the rotary knob back to "0".

03 Short-time operation

- Set the rotary knob to the desired cleaning duration.
- The timer switches off automatically after the time has expired. By turning the knob back, the cleaning duration can be shortened or the device can be switched off.

04 Information about the clock:

In a switched off status, the device can remain connected to the mains. A disconnection from the mains is achieved by unplugging the mains plug.



We recommend the RUCK® instrument disinfection item no.: 2940101 (2L) / 2940102 (5L)
and RUCK® instrument disinfection plus item no.: 2940901 (2L) / 2940902 (5L)
as well as the RUCK® ultrasonic cleaner item no.: 2944301



RUCK®
FÜR FUSS UND PFLEGE

Official representative:
Foot Care Center OÜ
Ahtri 6a, Tallinn 10151
+372 5644125
info@footcare.ee
www.jalakaubamaja.ee